

Approved by Director: Dr. Guy Vallaro

A. PURPOSE:

To use as a comprehensive guide in determining what serological tests are available and in what order they may be performed.

B. RESPONSIBILITY:

Forensic Science Examiners from the Connecticut State Forensic Science Laboratory who have been trained in the discipline of physical evidence examination according to SOP-FB-31 (Training Manual).


D. DEFINITIONS:

1. KM: Kastle-Meyer Test
2. OT: o-Tolidine Test

Approved by Director: Dr. Guy Vallaro

E. PROCEDURE:

Bloodstain Analysis

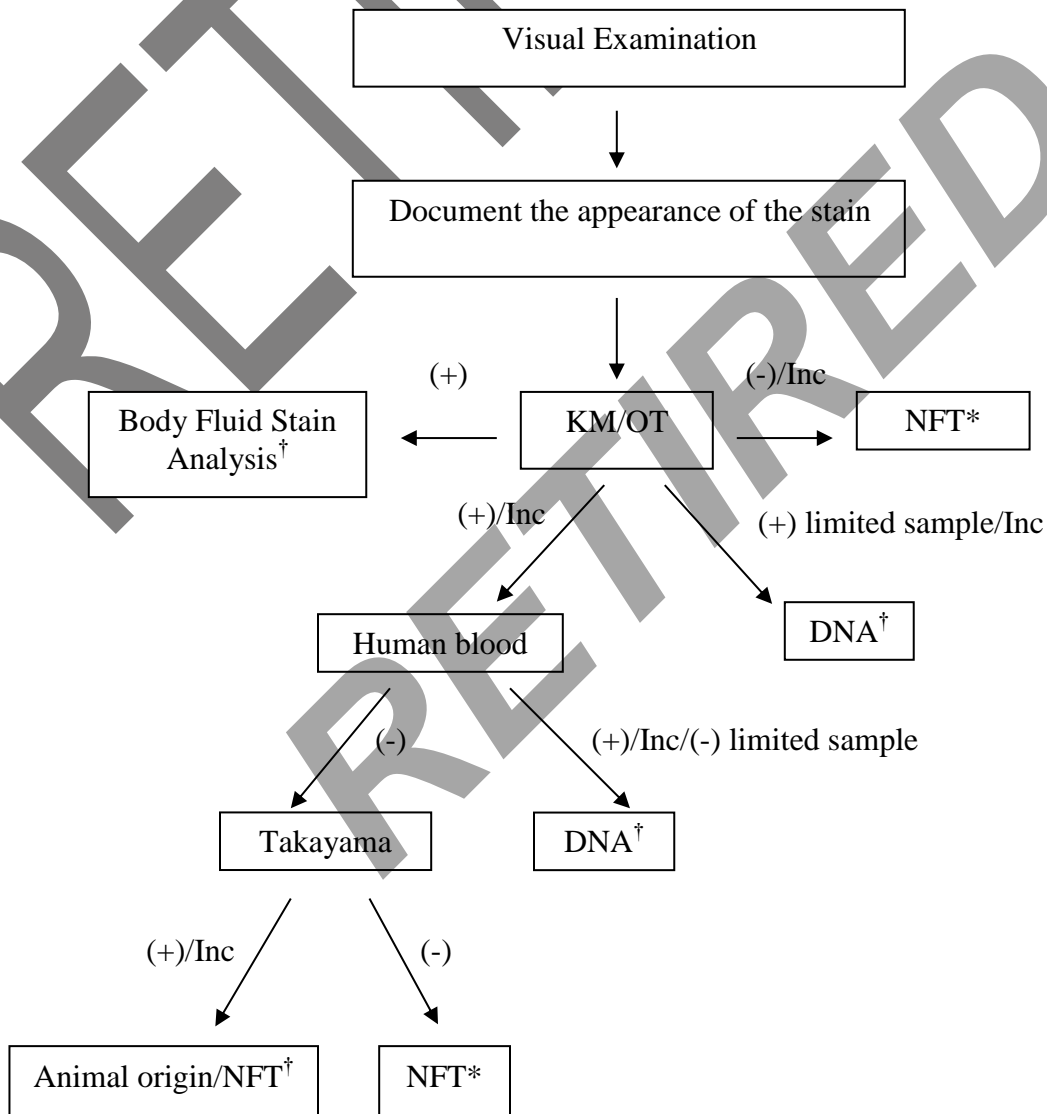


*NFT = No Further Testing

Approved by Director: Dr. Guy Vallaro

†Evaluation on a case-by-case basis
Inc=Inconclusive

Body Fluid Stain Analysis

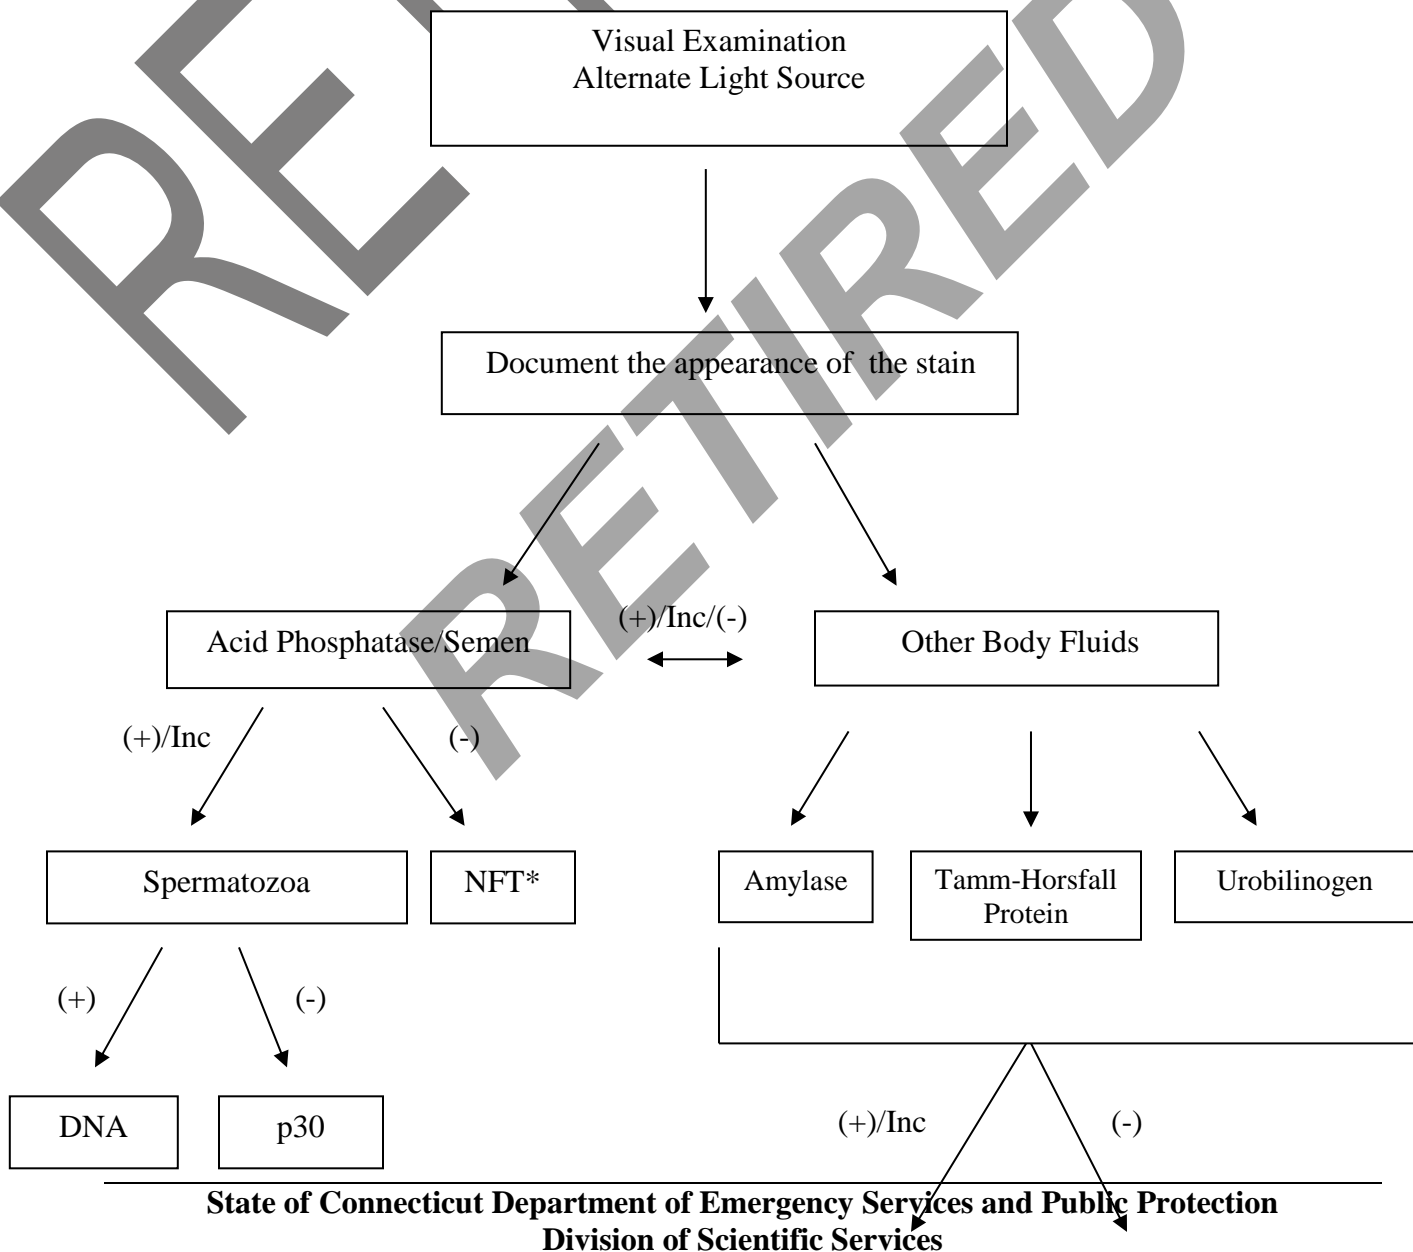

Documents outside of Qualtrax are considered uncontrolled.

FB SOP-03 Flow Charts

Document ID: 1338

Revision: 1

Effective Date: 8/19/2014

Status: Retired

Page 4 of 4

Approved by Director: Dr. Guy Vallaro



*NFT=No Further Testing

†Evaluation on a case-by-case basis

Inc=Inconclusive